



Fig. 1

1/20

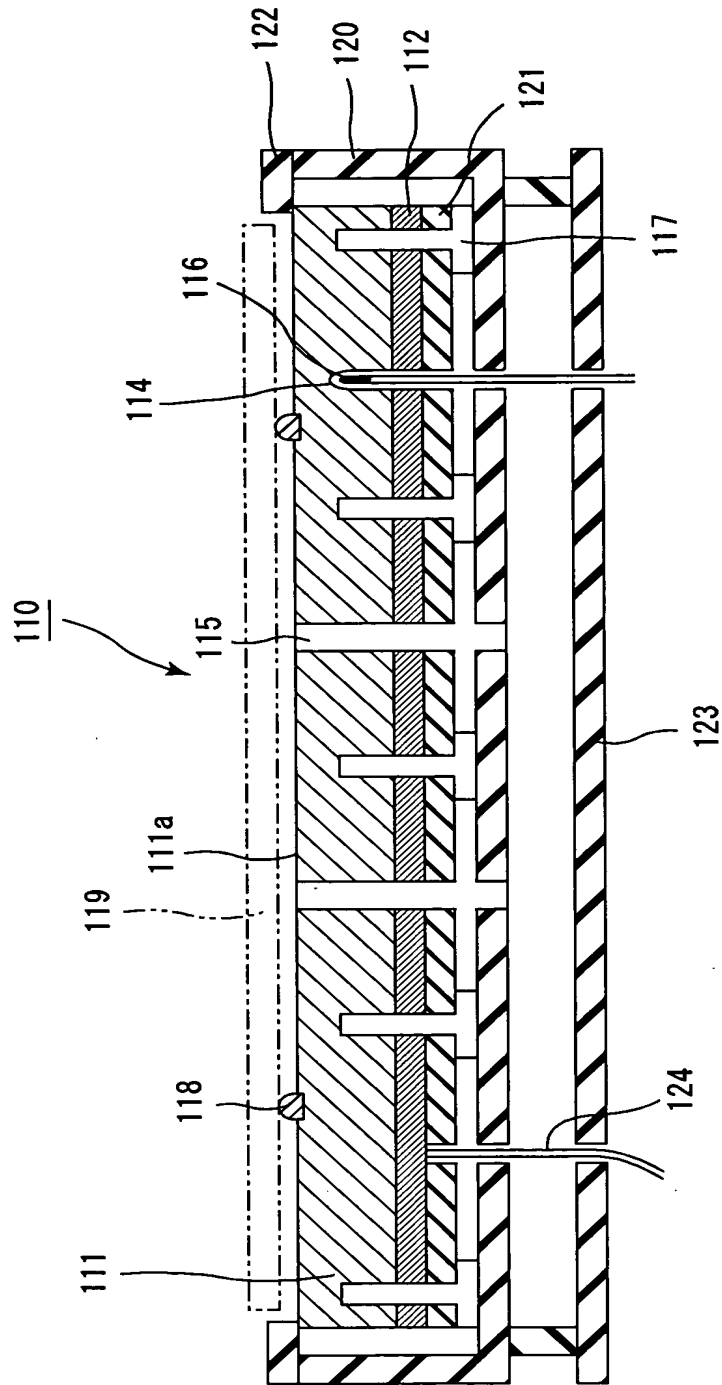


2/20

Fig. 2

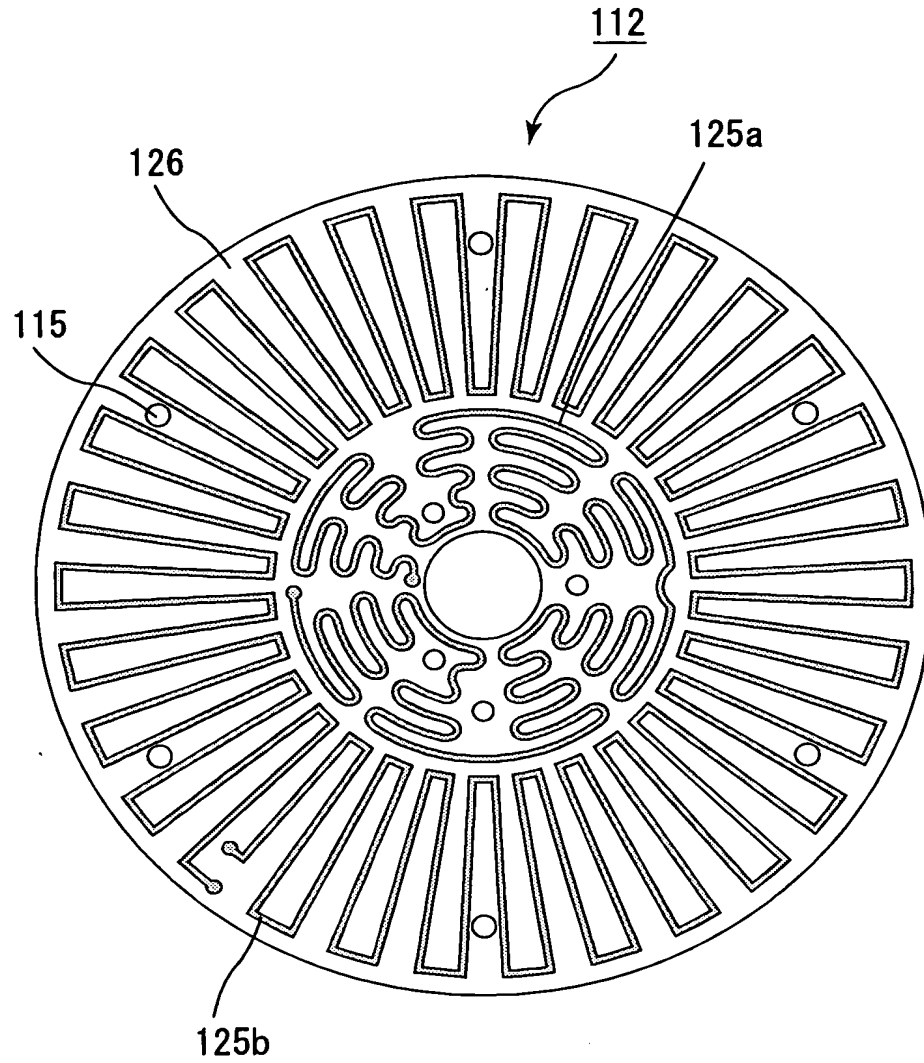


3/20

Fig. 3

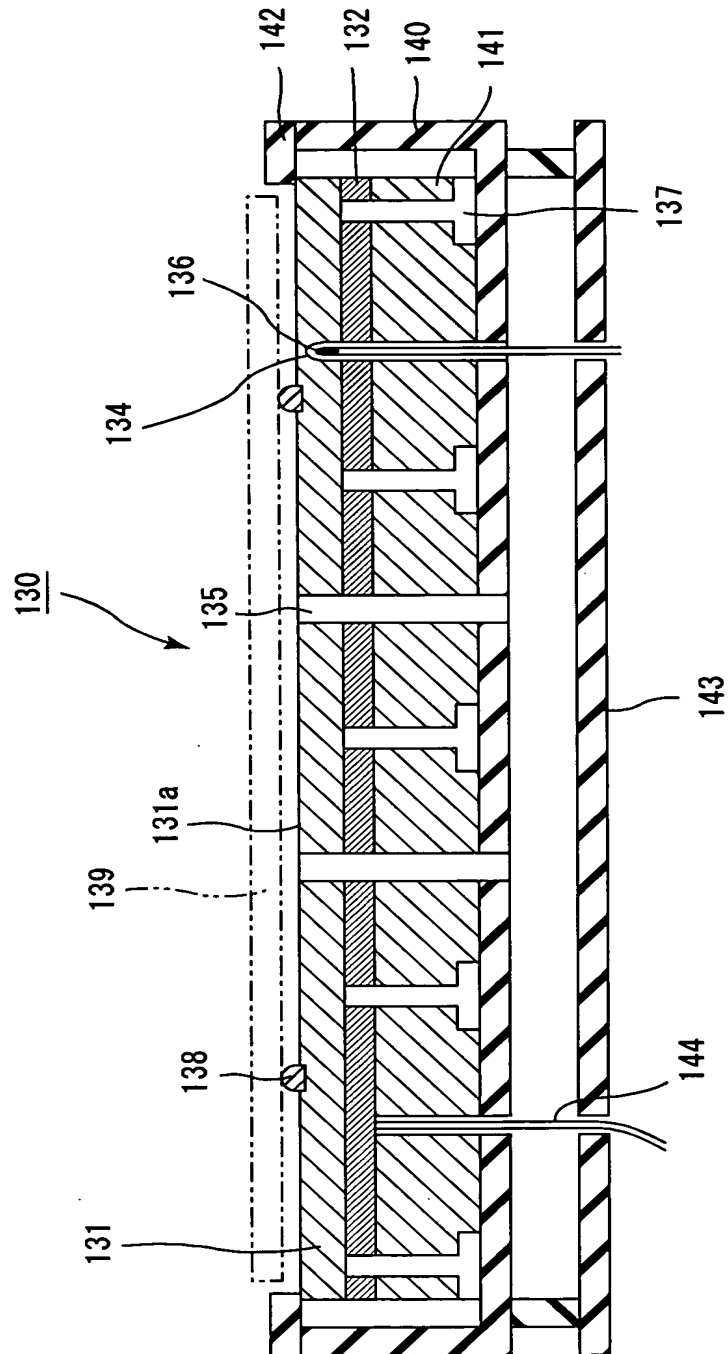

5/20


Fig. 5

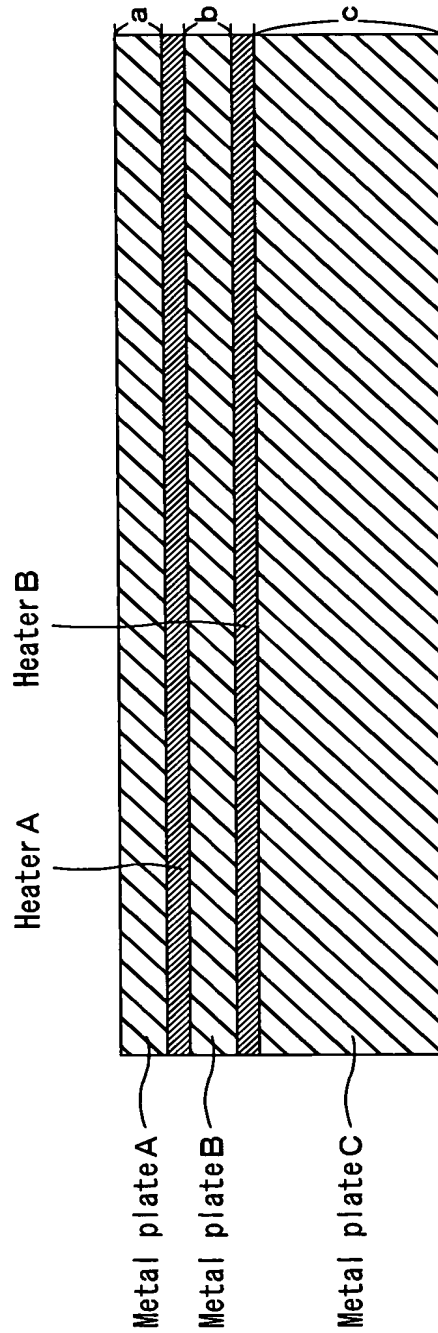

6/20

Fig. 6


MAX	140.16
MIN	139.91
AVE	140.03
RANGE	0.24

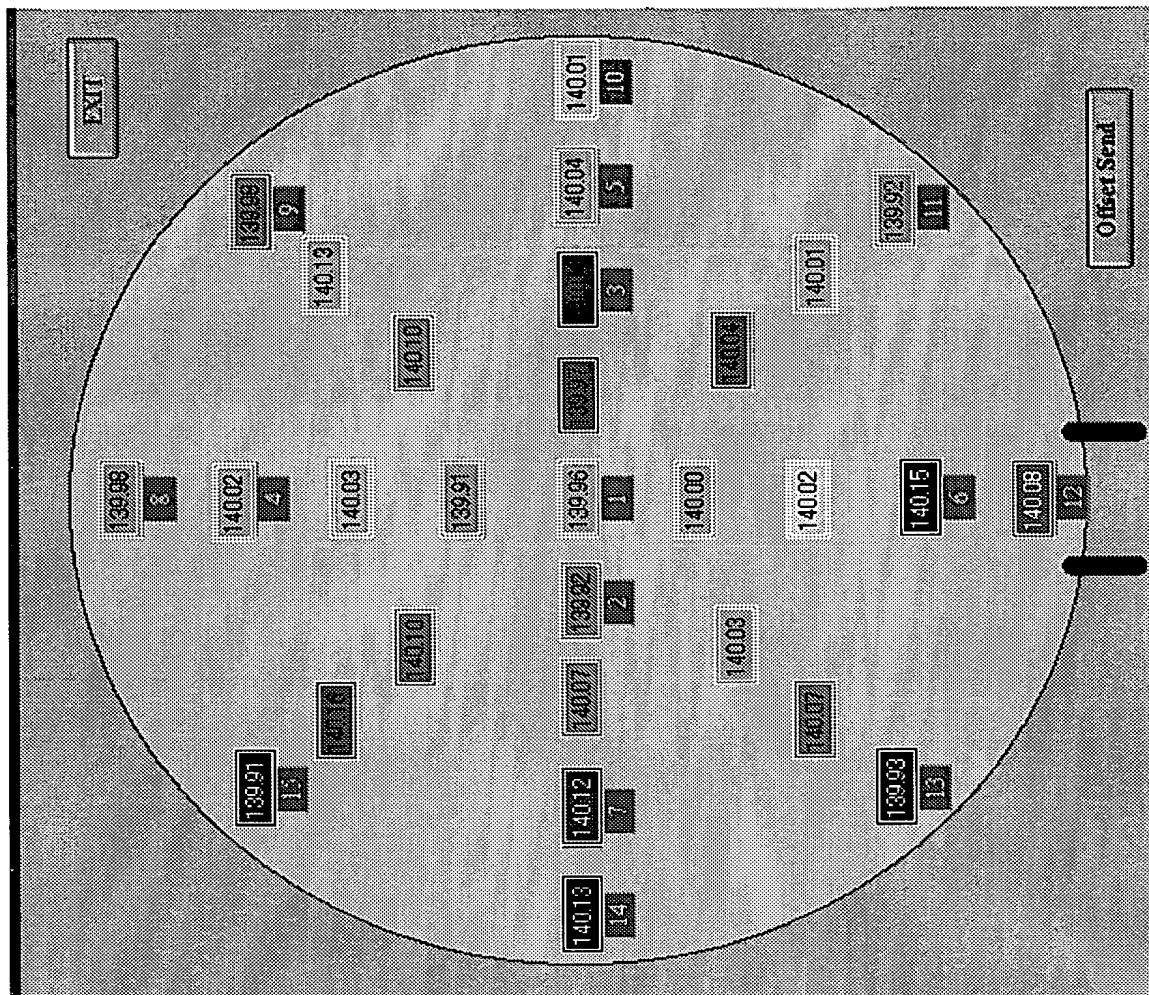

7/20


Fig. 7

MAX	140.28
MIN	139.61
AVE	139.97
RANGE	0.67

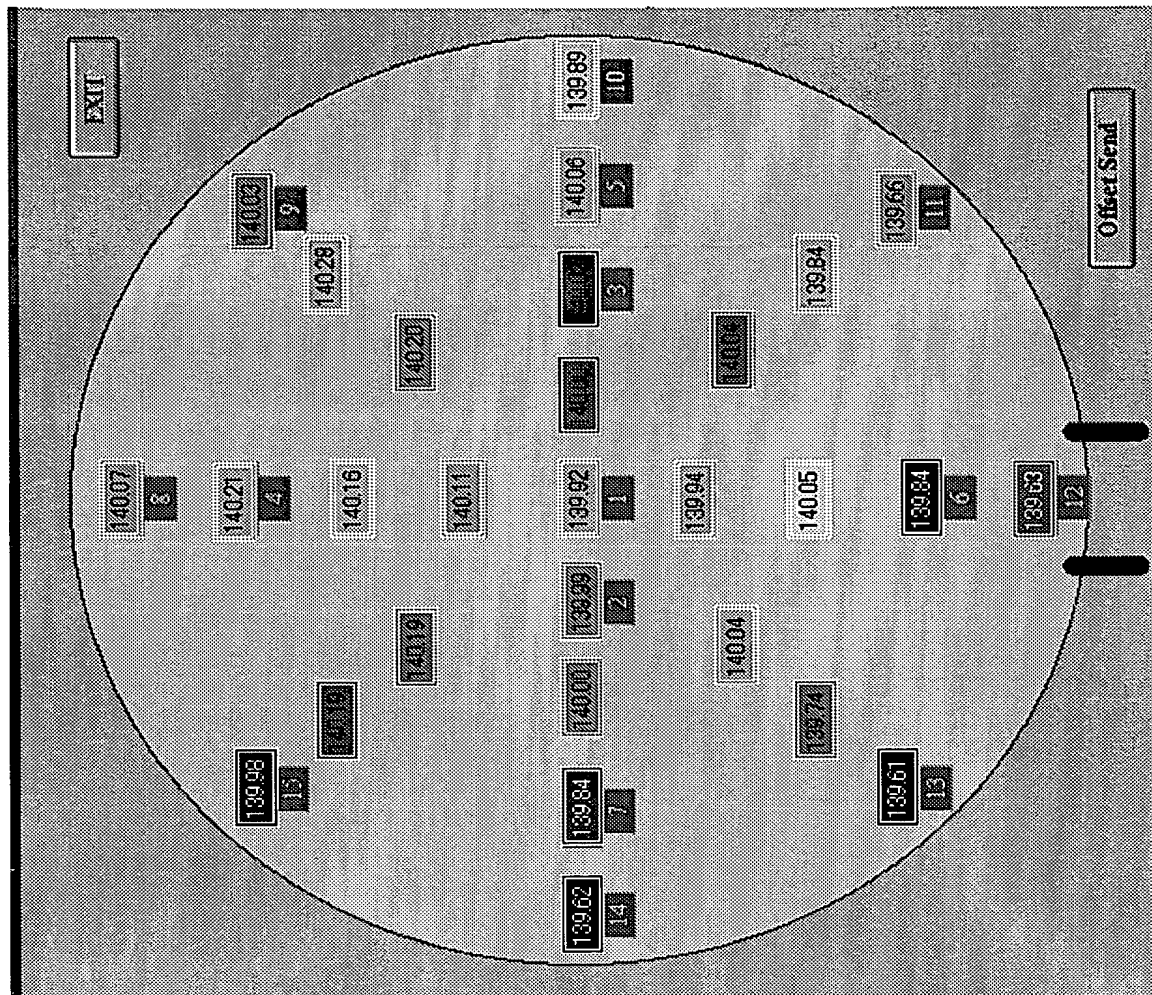


8/20

Fig. 8

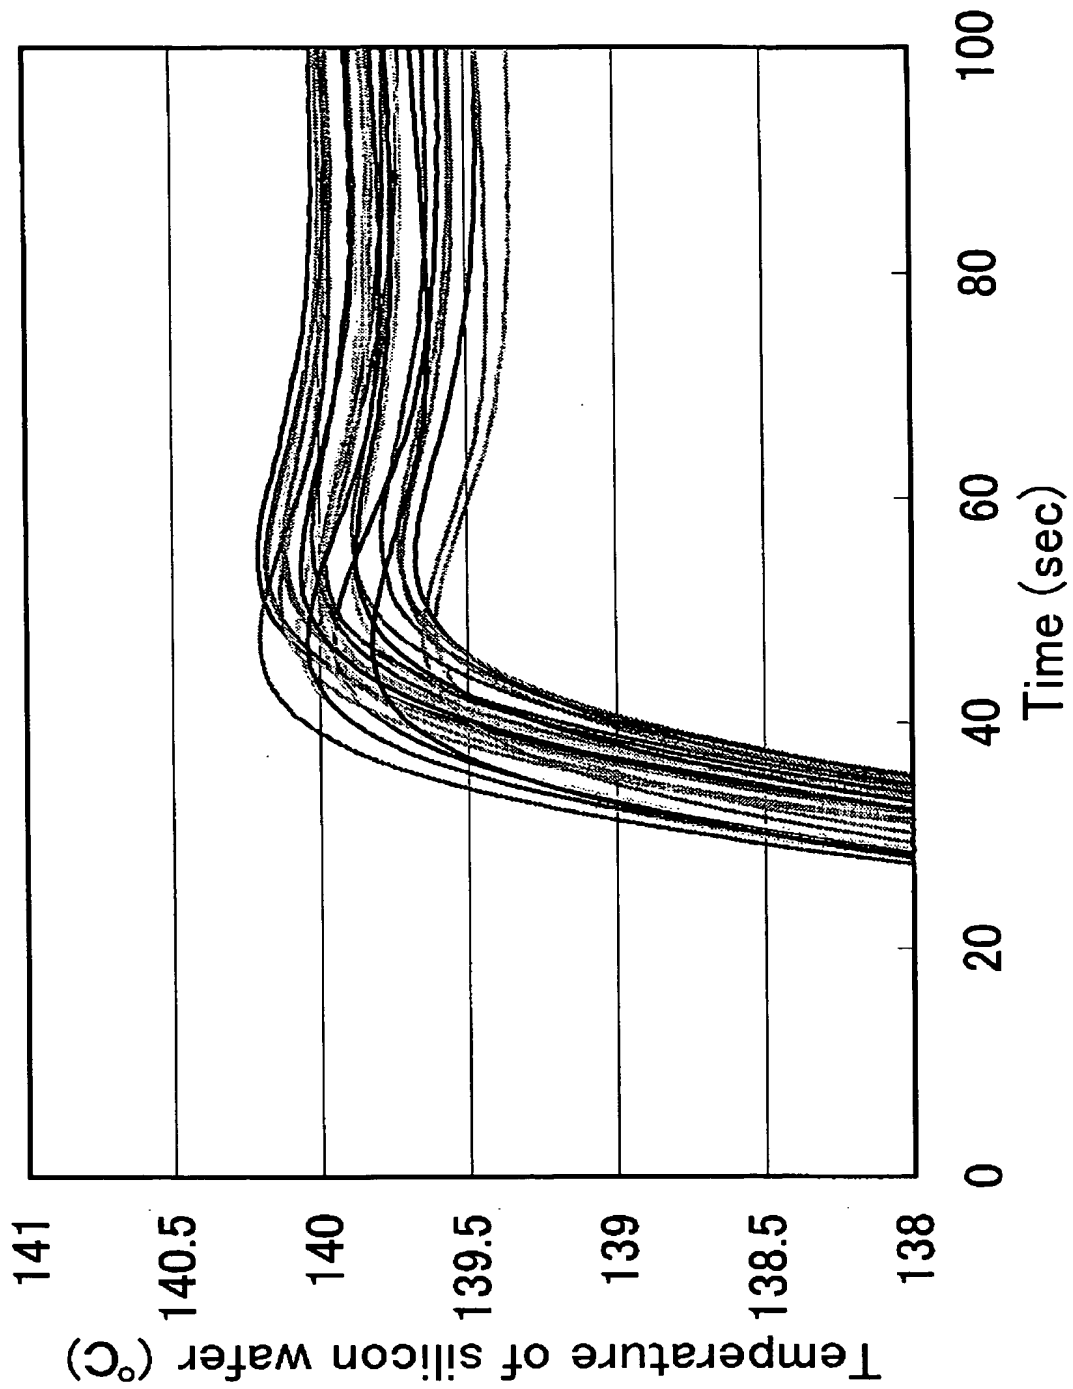


9/20

Fig. 9

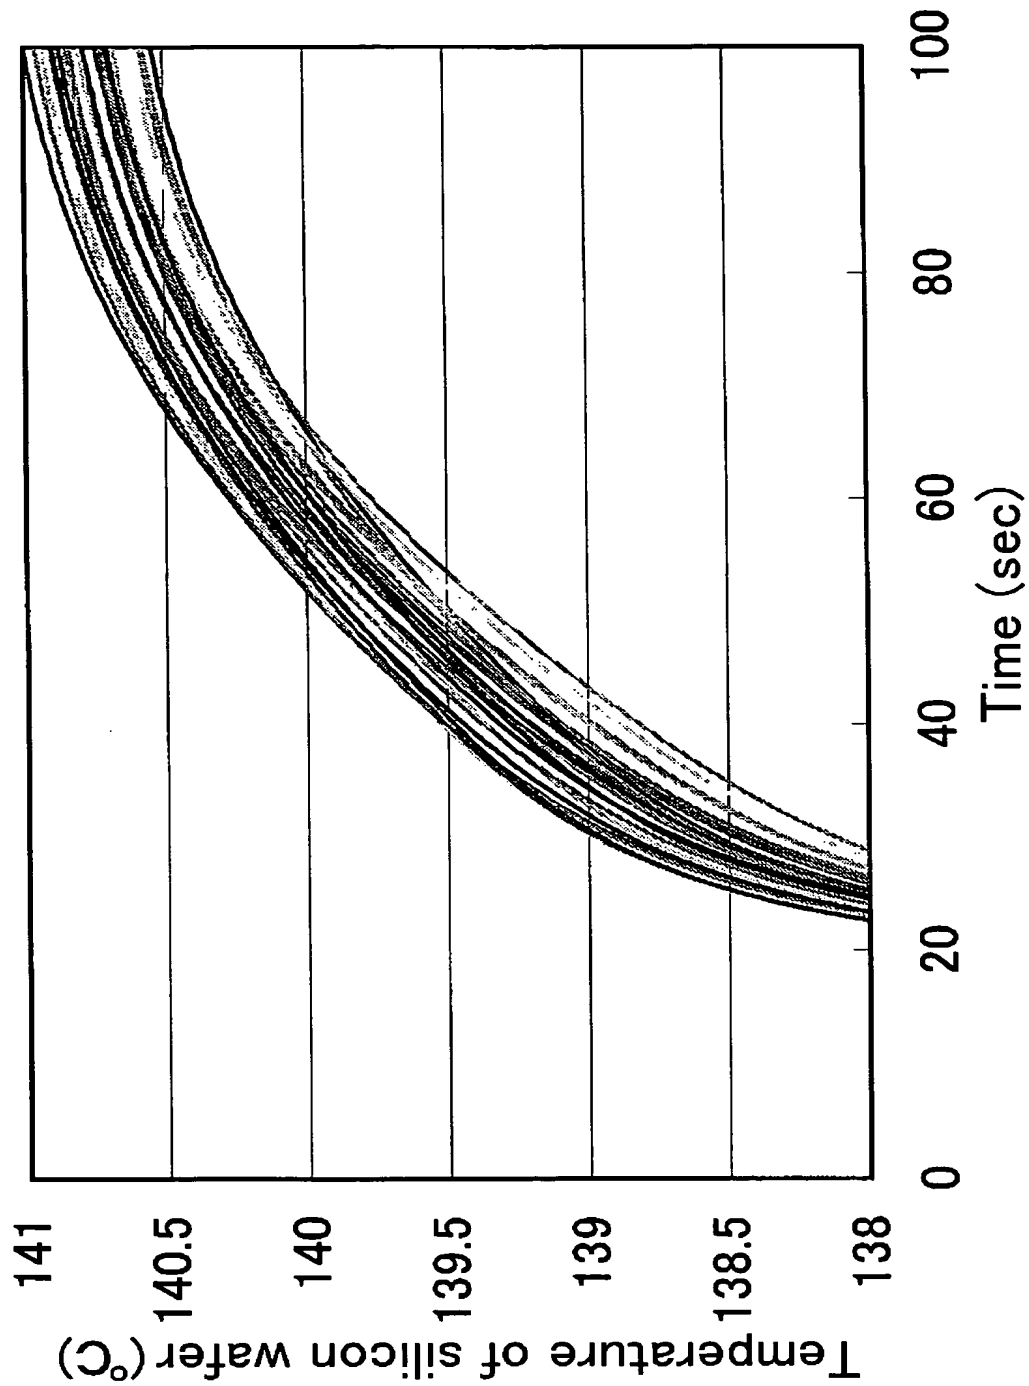


10/20

Fig. 10

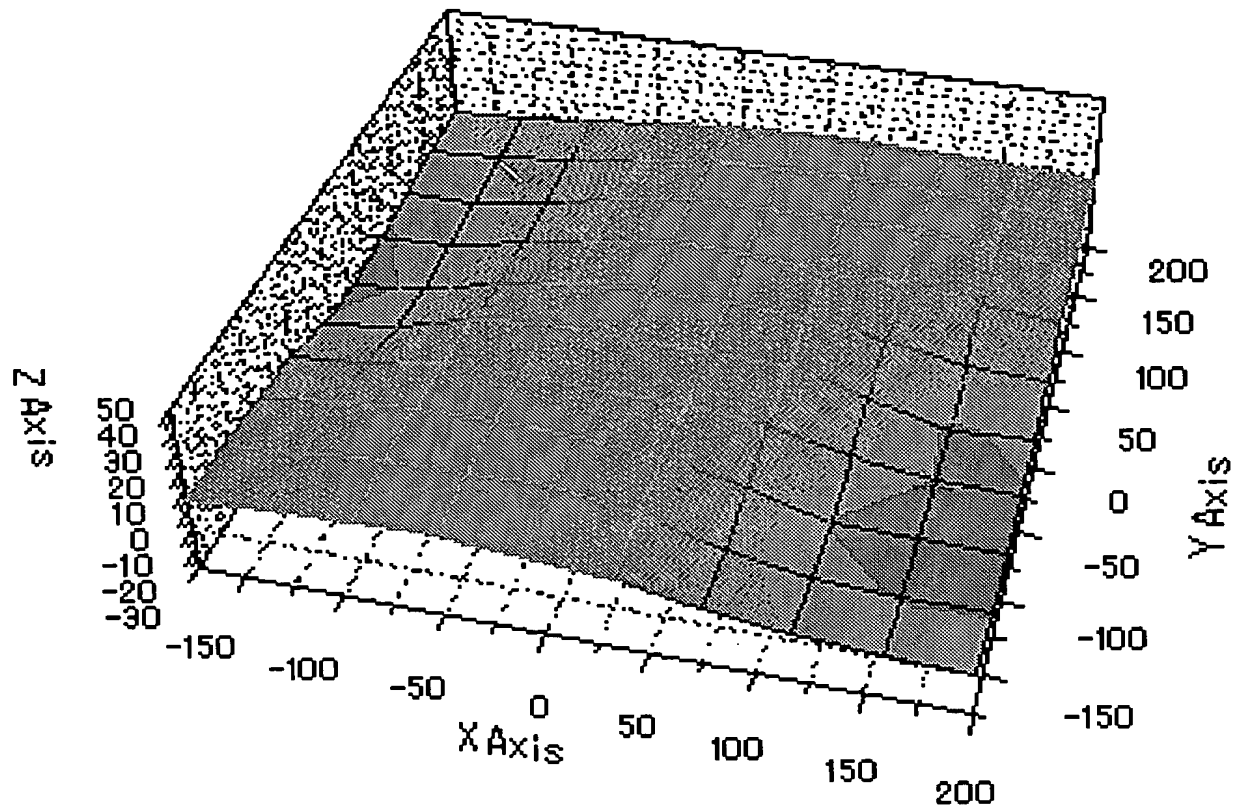


11/20

Fig. 11

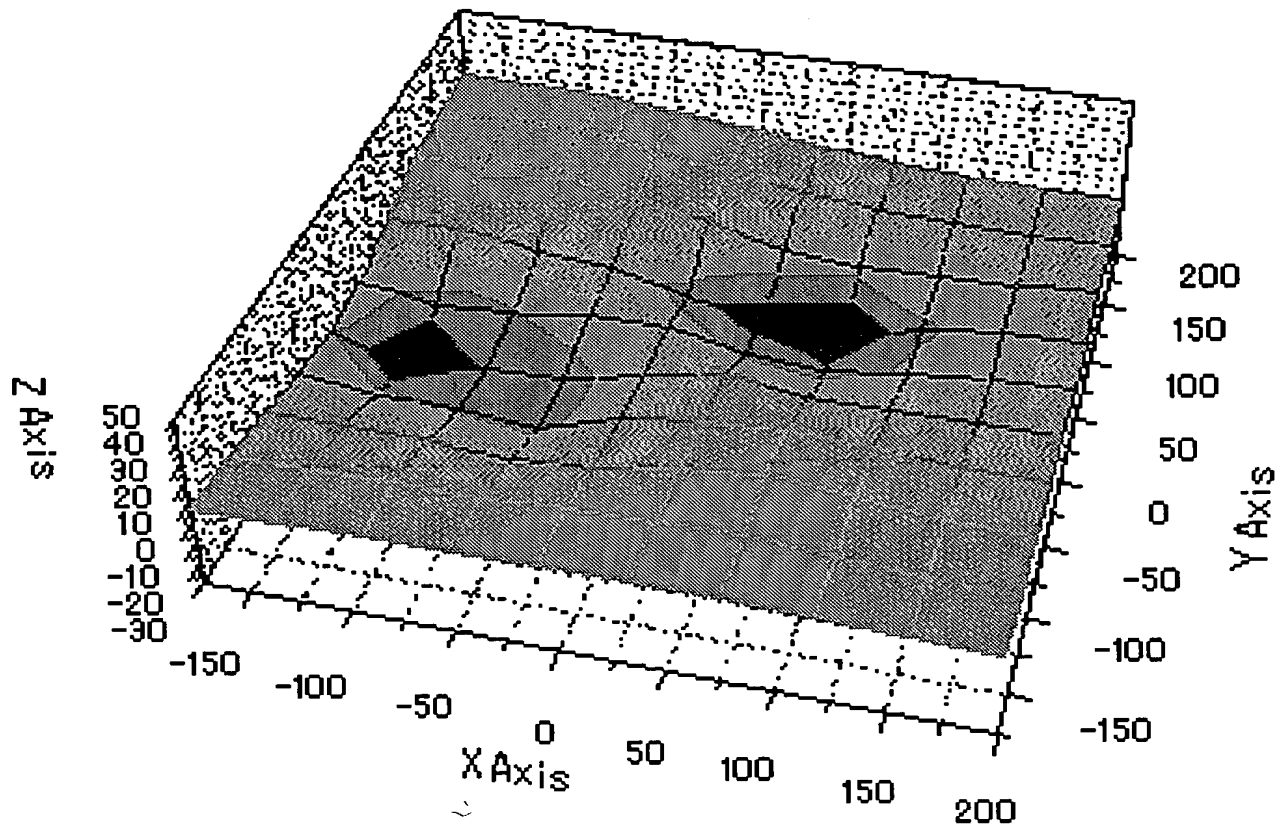


12/20

Fig. 12

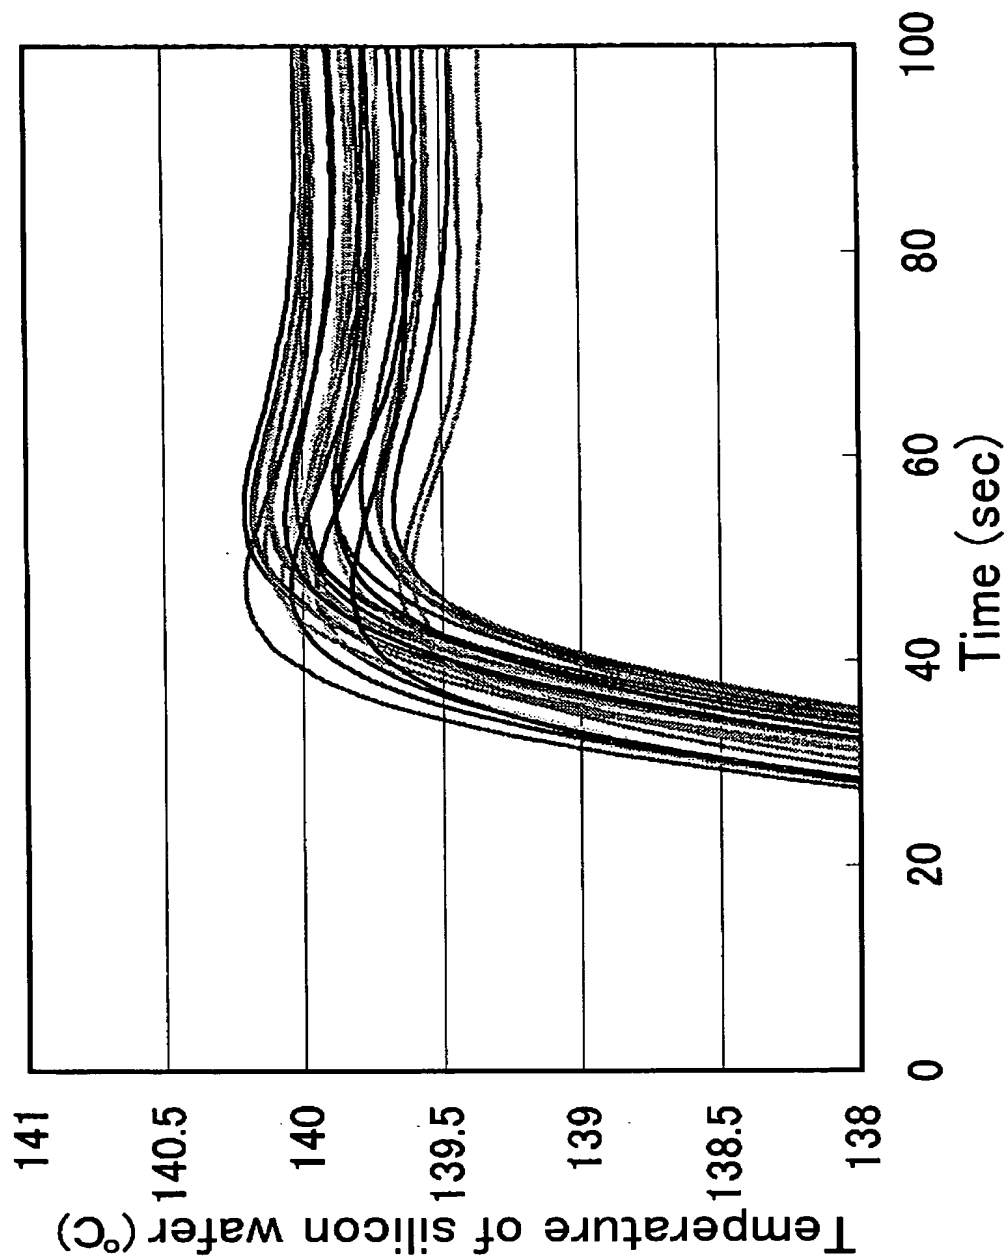


13/20

Fig. 13

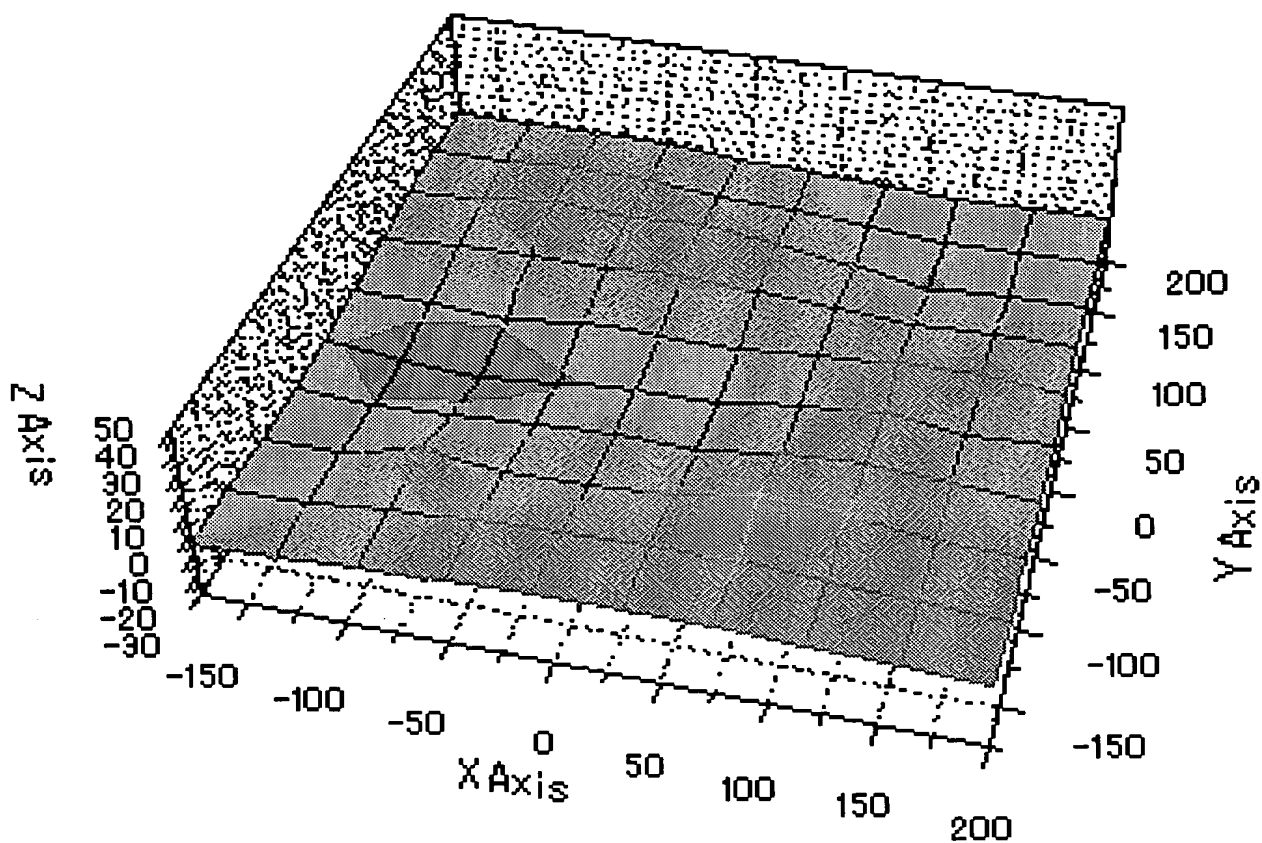

14/20


Fig. 14

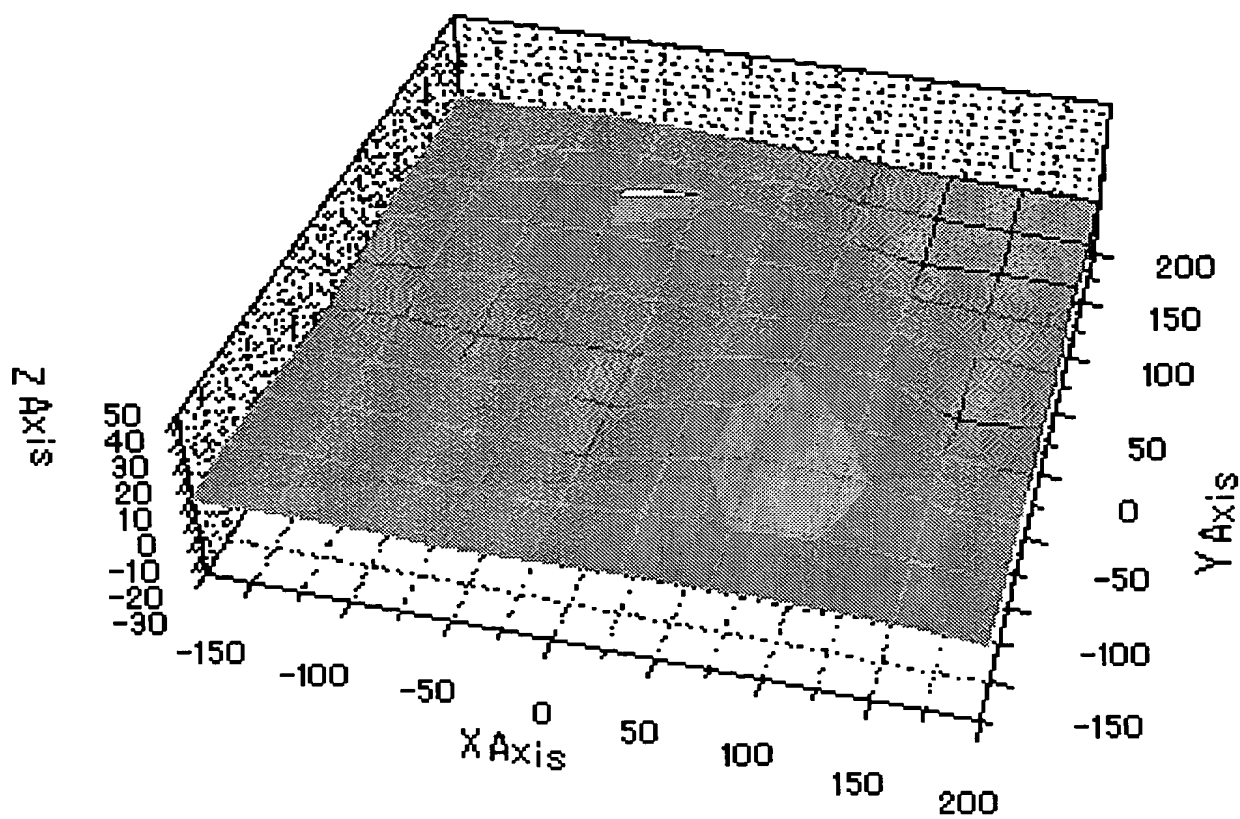

15/20

Fig. 15


MAX	140.09
MIN	139.80
AVE	139.96
RANGE	0.29

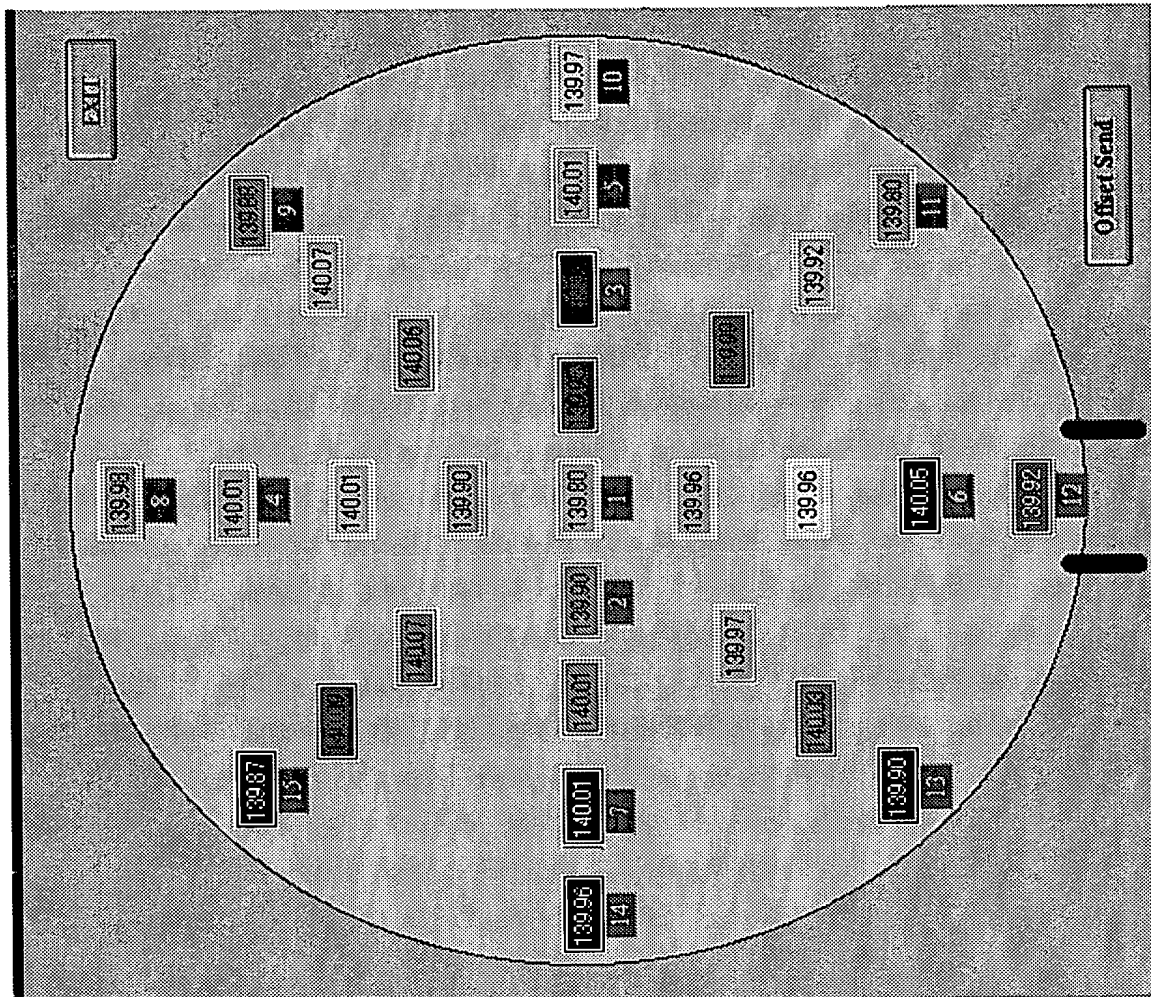

16/20


Fig. 16

MAX	140.22
MIN	139.57
AVE	139.95
RANGE	0.66

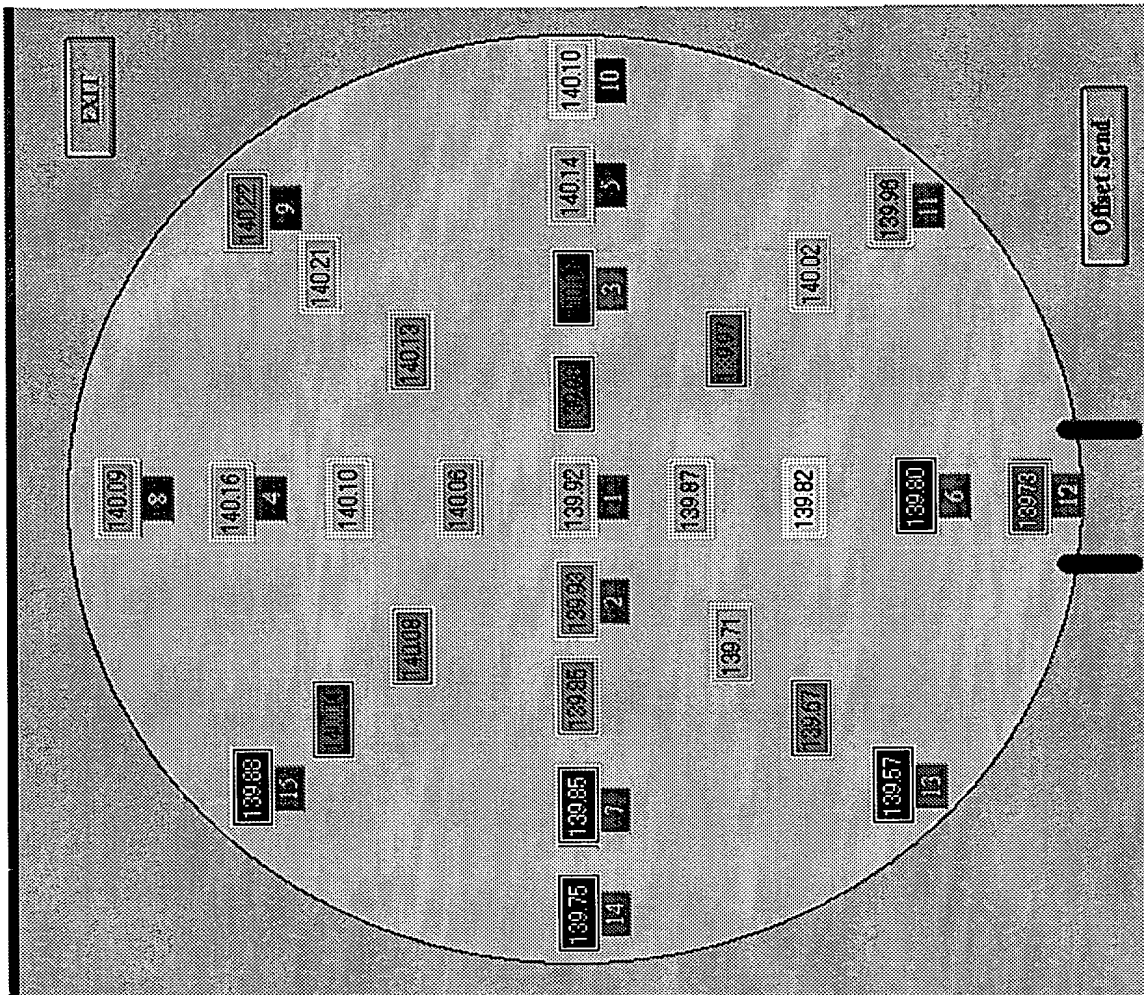


17/20

Fig. 17

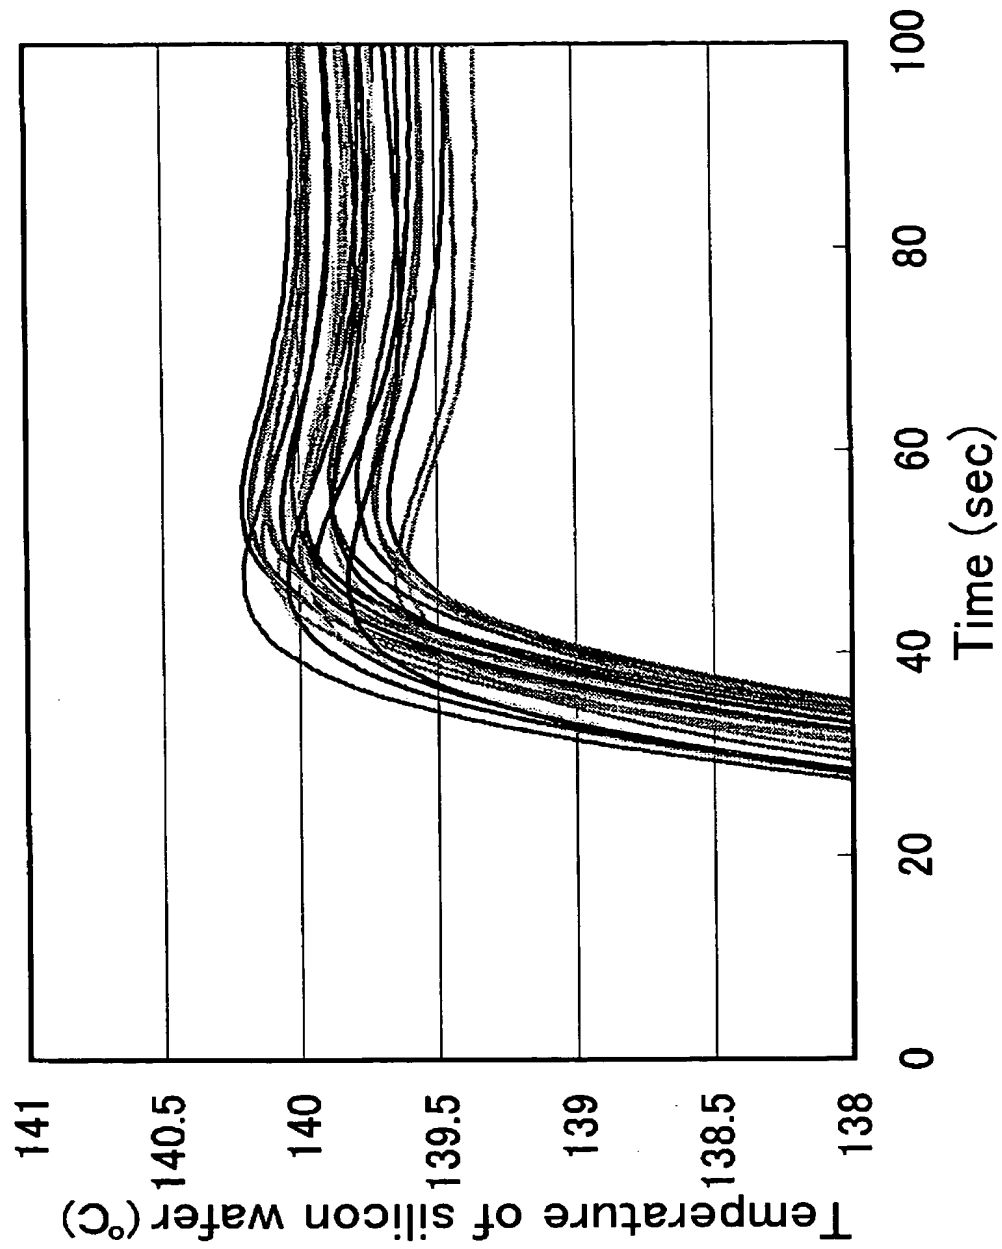


18/20

Fig. 18

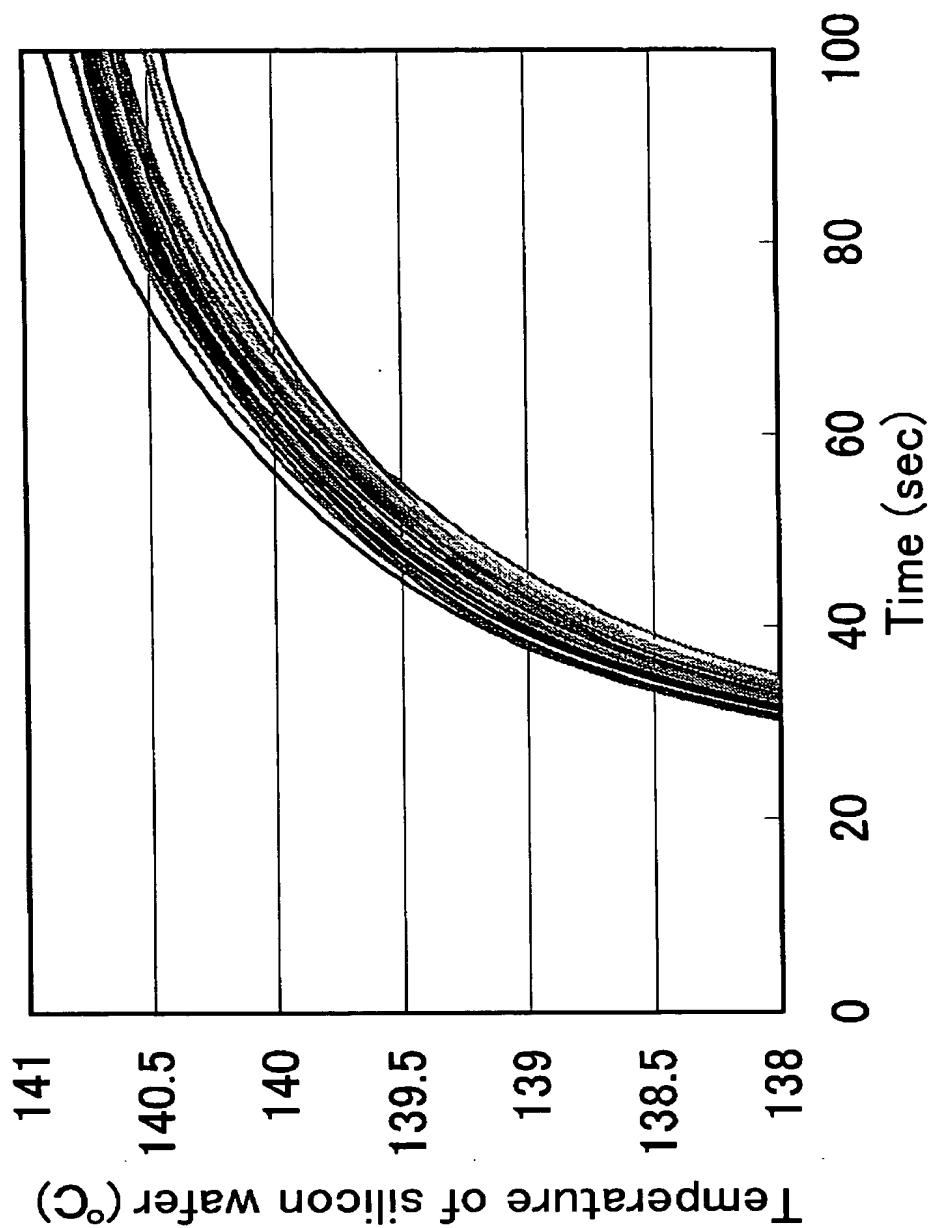

19/20

Fig. 19

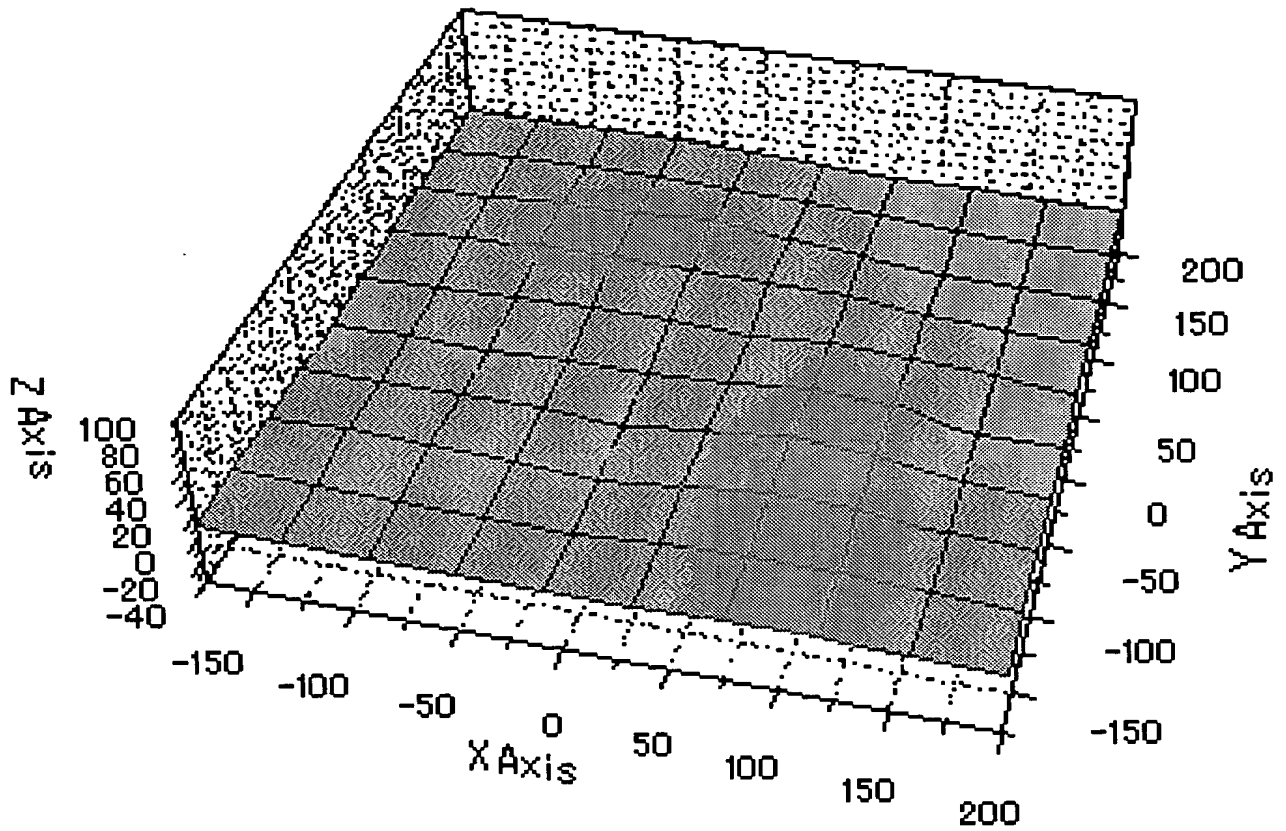

20/20

Fig. 20

